

KAMIYA BIOMEDICAL COMPANY

Dog Ceruloplasmin ELISA

For the quantitative determination of ceruloplasmin in dog serum or plasma

Cat. No. KT-1875

For Research Use Only.

PRODUCT INFORMATION

Dog Ceruloplasmin ELISA **Cat. No. KT-1875**

PRODUCT

The **K-ASSAY®** Dog Ceruloplasmin ELISA is an enzyme immunoassay for the quantitative determination of ceruloplasmin in dog serum or plasma. For research use only.

INTRODUCTION

Ceruloplasmin is an acute phase protein that is elevated in serum following injury, infection or disease. Studies indicate that ceruloplasmin levels increase up to 3-fold during the acute phase response in dogs.

PRINCIPLE

The **K-ASSAY®** Dog Ceruloplasmin ELISA uses affinity purified anti-dog ceruloplasmin for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated anti-dog ceruloplasmin for detection. Samples are diluted and incubated alongside calibrators in the microtiter wells for 45 minutes. The wells are subsequently washed and HRP conjugate is added and incubated for 45 minutes. Ceruloplasmin molecules, if present, are sandwiched between the immobilization and HRP-conjugated detection antibodies. The wells are then washed to remove unbound HRP-conjugate and TMB Reagent is added and incubated for 20 minutes at room temperature. This results in the development of a blue color. Color development is stopped by the addition of Stop Solution, changing the color to yellow, and absorbance is measured at 450 nm. The concentration of ceruloplasmin is proportional to the absorbance of the test sample and is determined from a calibration curve.

COMPONENTS

- Anti-dog ceruloplasmin coated 96 well plate (12 x 8-well strips)
- HRP-conjugate, 11 mL
- Ceruloplasmin stock (lyophilized)
- 10X Diluent, 25 mL
- 20X Wash Solution, 50 mL
- TMB Reagent, 11 mL
- Stop solution, 11 mL

MATERIALS REQUIRED BUT NOT PROVIDED

- Precision pipettors and tips.
- Distilled or de-ionized water.
- Microcentrifuge tubes.
- Vortex mixer.
- Absorbent paper or paper towels.
- Micro-Plate incubator/shaker with an approximate mixing speed of 150 rpm.
- Plate reader capable of measuring at 450 nm.
- Graphing software.

GENERAL INSTRUCTIONS

All reagents should be allowed to reach room temperature (25°C) before use.

Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of the instructions and with adherence to good laboratory practice.

The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

DILUENT PREPARATION

The diluent is provided as a 10X stock. Prior to use estimate the final volume of diluent required for your assay and dilute one (1) volume of the 10X stock with nine (9) volumes of distilled or de-ionized water.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20X stock. Prior to use dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water.

CALIBRATOR PREPARATION

1. The dog ceruloplasmin calibrator is provided as a lyophilized stock. Add the volume of distilled or de-ionized water indicated on the vial label and mix gently until dissolved.
2. Label 5 microcentrifuge tubes as 100, 50, 25, 12.5 and 6.25 ng/mL.
3. In the tube labeled 100 ng/mL, prepare the 100 ng/mL calibrator as described on the stock vial label.
4. Dispense 250 μ L of diluent into the tubes labeled 50, 25, 12.5 and 6.25 ng/mL.
5. Prepare the 50 ng/mL calibrator by diluting and mixing 250 μ L of the 100 ng/mL calibrator with 250 μ L of diluent in the appropriate tube.
6. Similarly prepare the 25, 12.5 and 6.25 ng/mL calibrators by 2-fold serial dilution.

Note: The reconstituted calibrator should be aliquoted and frozen at -20°C after reconstitution if further use is intended.

SAMPLE PREPARATION

Studies indicate that ceruloplasmin is present in dog serum at concentrations ranging from 100 to 400 μ g/mL. To obtain values within the range of the calibration curve we suggest that samples initially be diluted 10,000-fold using the following procedure.

1. Dispense 198 μ L and 297 μ L of diluent into separate tubes.
2. Pipette and mix 2 μ L of the serum/plasma sample into the tube containing 198 μ L of diluent. This provides a 100-fold diluted sample.
3. Mix 3 μ L of the 100-fold diluted sample with the 297 μ L of diluent in the second tube. This provides a 10,000-fold dilution of the sample.
4. Repeat this procedure for each sample to be tested.

ASSAY PROCEDURE

1. Secure the desired number of coated wells in the holder. Unused strips should be stored in the re-sealed bag with desiccant at 4°C for future use.
2. Dispense 100 μ L of calibrators and samples into the wells (we recommend that calibrators and samples be run in duplicate).
3. Incubate on an orbital micro-plate shaker at 100-150 rpm and 25°C for 45 minutes.
4. Empty and wash the microtiter wells 5x with 1X wash solution using a plate washer (400 μ L/well).
5. Strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.
6. Add 100 μ L of HRP-conjugate reagent into each well.
7. Incubate on a plate shaker at 100-150 rpm and 25°C for 45 minutes.
8. Wash as detailed above.
9. Strike the wells sharply onto absorbent paper or paper towels to remove all residual droplets.
10. Dispense 100 μ L of TMB reagent into each well.
11. Incubate on an orbital micro-plate shaker at 100-150 rpm at 25°C for 20 minutes.
12. After 20 minutes, stop the reaction by adding 100 μ L of Stop solution to each well.
13. Gently mix. It is important to make sure that all the blue color changes to yellow.
14. Read absorbance at 450 nm with a plate reader within 5 minutes.

CALCULATION OF RESULTS

1. Use graphing software to construct a calibration curve by plotting the absorbance values for each calibrator versus its concentration in ng/mL, with absorbance values on the Y-axis and concentrations on the X-axis.
2. Fit the data using a single-site, total and non-specific binding model.
3. Determine the concentration of ceruloplasmin in ng/mL from the calibration curve.
4. Multiply the derived concentration by the dilution factor to determine the concentration of ceruloplasmin in the


serum/plasma sample.

5. If the A_{450} values of samples fall outside the calibration curve when tested at a 10,000-fold dilution, samples should be diluted appropriately and re-tested.

TYPICAL CALIBRATION CURVE

A typical calibration curve is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns. Each user should obtain his or her data and calibration curve in each experiment.

Ceruloplasmin (ng/mL)	A_{450}
100	2.896
50	1.859
25	1.049
12.5	0.558
6.25	0.377

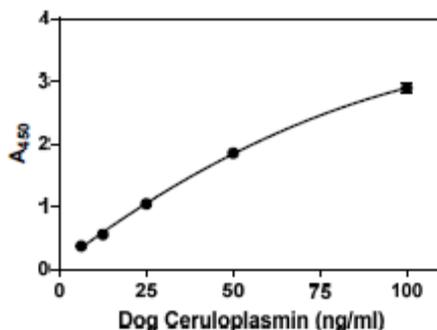

STORAGE

The kit should be stored at 4°C and the microtiter plate should be kept in a sealed bag with desiccant to minimize exposure to damp air. The expiration date of the kit is indicated on the box label.

FOR RESEARCH USE ONLY

KAMIYA BIOMEDICAL COMPANY

12779 Gateway Drive, Seattle, WA 98168
 Tel: (206) 575-8068 Fax: (206) 575-8094
 Email: LifeScience@k-assay.com
 www.k-assay.com