

KAMIYA BIOMEDICAL COMPANY

Sheep C-Reactive Protein (CRP) ELISA

For the quantitative determination of CRP in sheep serum and plasma

Cat. No. KT-786

For Research Use Only.

PRODUCT INFORMATION

Sheep C-Reactive Protein (CRP) ELISA Cat. No. KT-786

PRODUCT

The **K-ASSAY®** Sheep C-Reactive Protein (CRP) ELISA is an enzyme immunoassay for the quantitative determination of CRP in sheep serum and plasma. For research use only.

INTRODUCTION

CRP is an acute phase protein that is elevated in serum from most mammals as a result of infection and disease and can be used as a biomarker to evaluate health status.

PRINCIPLE

The **K-ASSAY®** Sheep C-Reactive Protein (CRP) ELISA is based on a solid phase enzyme-linked immunosorbent assay (ELISA). The assay uses affinity purified anti-sheep CRP antibodies for solid phase (microtiter wells) immobilization and horseradish peroxidase (HRP) conjugated anti-sheep CRP antibodies for detection. Diluted samples and calibrators are first incubated in the microtiter wells for 45 minutes. The wells are subsequently washed and HRP conjugate is added and incubated for 45 minutes. CRP molecules are thereby sandwiched between the immobilization and detection antibodies. The wells are washed to remove unbound HRP-labeled antibodies. TMB Reagent is then added and incubated for 20 minutes. This results in the development of a blue color if CRP is present in the sample. Color development is stopped by the addition of Stop Solution, changing the color to yellow. Absorbance is measured spectrophotometrically at 450 nm. The concentration of CRP is proportional to the absorbance and is derived from a calibration curve.

COMPONENTS

- Anti-sheep CRP antibody coated microtiter plate with 96 wells (provided as 12 detachable strips of 8)
- HRP Conjugate Reagent, 11 mL
- Sheep CRP Stock
- 10X Diluent, 25 mL
- 20X Wash Solution, 50 mL
- TMB Reagent (One-Step), 11 mL
- Stop Solution (1N HCl), 11 mL

MATERIALS REQUIRED BUT NOT PROVIDED

- Precision pipettes and tips
- Distilled or de-ionized water
- Polypropylene or glass tubes
- Vortex mixer
- Absorbent paper or paper towels
- Micro-Plate incubator/shaker with an approximate mixing speed of 150 rpm
- A microtiter plate reader at 450 nm wavelength with an optical density range of 0-4 OD
- Graph paper (PC graphing software is optional)

STORAGE

The unused kit should be stored at 4°C. The microtiter plate should be kept in a sealed bag with desiccant to minimize exposure to damp air. The kit will remain stable until the expiration date provided that the components are stored as described above.

GENERAL INSTRUCTIONS

All reagents used directly in the assay should be allowed to reach room temperature (25°C) before use.

DILUENT PREPARATION

The diluent is provided as a 10X stock. Prior to use estimate the final volume of diluent required for your assay and dilute one (1) volume of the 10X stock with nine (9) volumes of distilled or de-ionized water.

WASH SOLUTION PREPARATION

The wash solution is provided as a 20X stock. Prior to use dilute the contents of the bottle (50 mL) with 950 mL of distilled or de-ionized water.

CALIBRATOR PREPARATION

1. Reconstitute the lyophilized sheep CRP calibrator stock vial as described on the vial label. The reconstituted stock is stable for one day at 4°C but should be aliquoted and frozen $\leq -20^{\circ}\text{C}$ if future use is intended.
2. Label 6 polypropylene or glass tubes: 250, 125, 62.5, 31.25, 15.63 and 7.81 ng/mL.
3. Prepare a 250 ng/mL working CRP calibrator as detailed on the calibrator vial label by mixing the indicated volume of diluent and reconstituted stock in the tube labeled 250 ng/mL.
4. Dispense 250 μL of diluent into the tubes labeled 125, 62.5, 31.25, 15.63 and 7.81 ng/mL.
5. Prepare a 125 ng/mL calibrator by diluting and mixing 250 μL of the 250 ng/mL calibrator with 250 μL of diluent in the tube labeled 125 ng/mL. Similarly prepare the remaining calibrators by serial dilution.

SAMPLE PREPARATION

General Note: In studies, we found CRP levels ranging of approximately 90 $\mu\text{g}/\text{mL}$ in normal sheep serum. In order to obtain values within the range of the calibration curve we suggest that samples be diluted 2,000 fold initially using the following procedure for each sample:

1. Dispense 98 μL and 243.75 μL of 1X diluent into two separate tubes.
2. Pipette and mix 2.0 μL of the serum/plasma sample into the first tube. This provides a 50 fold diluted sample.
3. Mix 6.25 μL of the 50 fold diluted sample with the 243.75 μL of diluent in the second tube. This provides a 2,000 fold dilution of the sample.

ASSAY PROCEDURE

1. Secure the desired number of coated wells in the holder.
2. Dispense 100 μL of calibrators and diluted samples into the wells (we recommend that calibrators and samples be tested in duplicate).
3. Incubate on an orbital micro-plate shaker at 150 rpm at room temperature (25°C) for 45 minutes.
4. Aspirate the contents of the microtiter wells and wash the wells 5 times with 1X wash solution using a plate washer (400 $\mu\text{L}/\text{well}$). The entire wash procedure should be performed as quickly as possible.
5. Strike the wells sharply onto adsorbent paper or paper towels to remove all residual droplets.
6. Add 100 μL of enzyme conjugate reagent into each well.
7. Incubate on an orbital micro-plate shaker at 150 rpm at room temperature (25°C) for 45 minutes.
8. Wash as detailed in 4 and 5 above.
9. Dispense 100 μL of TMB Reagent into each well.
10. Gently mix on an orbital micro-plate shaker at 150 rpm at room temperature (25°C) for 20 minutes.
11. Stop the reaction by adding 100 μL of Stop Solution to each well.
12. Gently mix. It is important to make sure that all the blue color changes to yellow.
13. Read the optical density at 450 nm with a microtiter plate reader within 15 minutes.


CALCULATION OF RESULTS

1. Calculate the average absorbance values (A_{450}) for each set of reference calibrators and samples.
2. Construct a calibration curve by plotting the mean absorbance obtained from each reference calibrator against its concentration in ng/mL on linear graph paper, with absorbance values on the vertical or Y-axis and concentrations on the horizontal or X-axis.
3. Using the mean absorbance value for each sample, determine the corresponding concentration of CRP in ng/mL from the calibration curve.
4. Multiply the derived concentration by the dilution factor to determine the actual concentration of CRP in the serum/plasma sample.
5. If available, PC graphing software should be used for the above steps. We recommend a second order polynomial fit for the calibration curve.
6. If the OD_{450} values of samples fall outside the calibration curve when tested at a 2,000 fold dilution, samples should be diluted appropriately and re-tested.

TYPICAL CALIBRATION CURVE

A typical calibration curve with optical density readings at 450 nm on the Y-axis against CRP concentrations on the X-axis is shown below. This curve is for the purpose of illustration only and should not be used to calculate unknowns. Each user should obtain his or her data and calibration curve in each experiment.

| CRP (ng/mL) | Absorbance (450 nm) |
|-------------|---------------------|
| 250 | 3.290 |
| 125 | 1.931 |
| 62.5 | 1.073 |
| 31.25 | 0.547 |
| 15.63 | 0.319 |
| 7.81 | 0.194 |

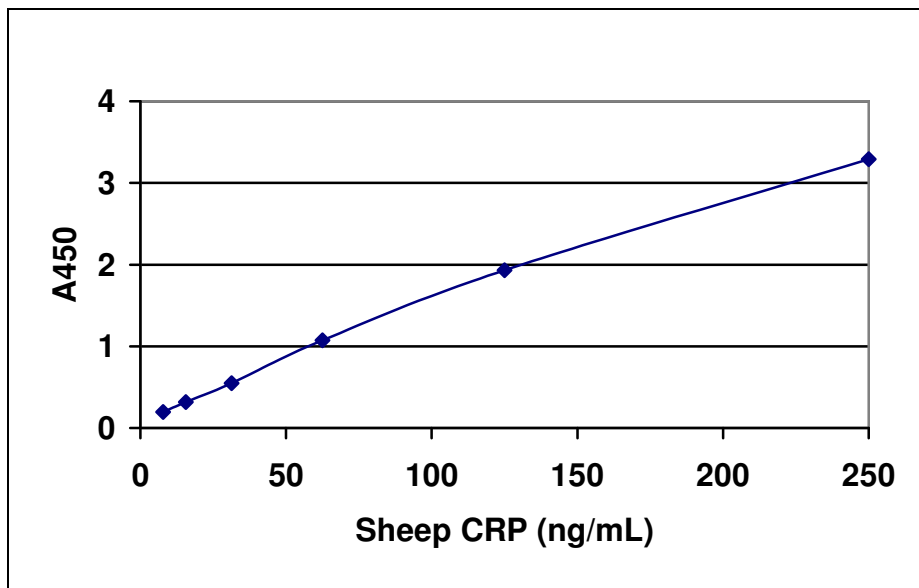

LIMITATIONS OF THE PROCEDURE

1. Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of the instructions and adherence to good laboratory practice.
2. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.

FOR RESEARCH USE ONLY

KAMIYA BIOMEDICAL COMPANY

12786 Gateway Drive, Seattle, WA 98168
 Tel: (206) 575-8068 Fax: (206) 575-8094
 Email: LifeScience@k-assay.com
 www.k-assay.com